

# PD24-03-PR Mid-Infrared Photodiodes

## Description


Photodiodes PD24-03-PR are fabricated from narrow band-gap GaInAsSb/AlGaAsSb-based heterostructures lattice matched to GaSb substrate, and are designed for detection of light signals in Mid-Infrared spectral range with cut-off wavelength around 2.4  $\mu\text{m}$ .

## Features

- Diameter of photosensitive area: 0.3 mm
- Fast Response: <50 ns
- Package: TO-18 with a parabolic reflector without a window

## Applications


- Industrial Process Control
- Sensor development
- Medical diagnostics

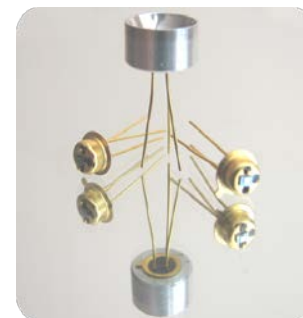

## Specification

### Recommended modes of PD operation

We recommend using photovoltaic mode, when PD is used under no reverse bias.

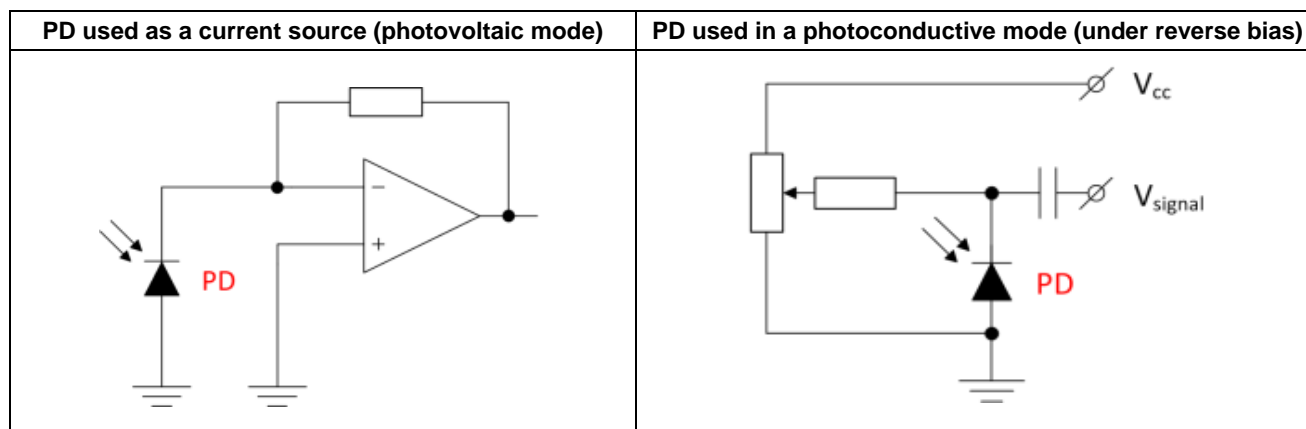

### Device Parameters


Device Parameters	Symbol	Value	Units
Sensitive area diameter	d	0.3	mm
Storage temperature	$T_{\text{stg}}$	-200 ~ +70	$^{\circ}\text{C}$
Operating temperature	$T_{\text{opr}}$	-200 ~ +60	$^{\circ}\text{C}$
Reverse voltage	$V_r$	-1	V

### Optical and Electrical Characteristics


Photodiode Parameters	Conditions	Symbol	Value	Units
Cut-off wavelength	T=300 K	$\lambda_{cut}$	2.4	$\mu\text{m}$
Max. sensitivity wavelength (>90%)	T=300 K	$\lambda_p$	1.85 — 2.3	$\mu\text{m}$
Dark current	T=300 K, $V_r=-1$ V	$I_d$	10 — 60	$\mu\text{A}$
Shunt resistance	T=300 K, $V_r=-10$ mV	$R_{sh}$	3 — 8	k $\Omega$
Capacitance	T=300 K, $\lambda=\lambda_p$	C	20 — 80	pF
Sensitivity	T=300 K, $\lambda=\lambda_p$	S	0.7-1.0	A/W
Detectivity	T=300 K, $\lambda=\lambda_p$	$D^*$	(1-4)* $10^{10}$	$\text{cm}\cdot\text{Hz}^{1/2}\cdot\text{W}^{-1}$

### Typical Characteristic Curves


Spectral response (typical)

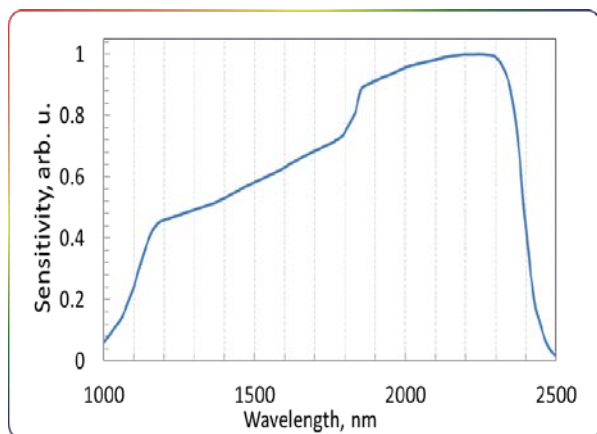


Temperature shift of spectral response

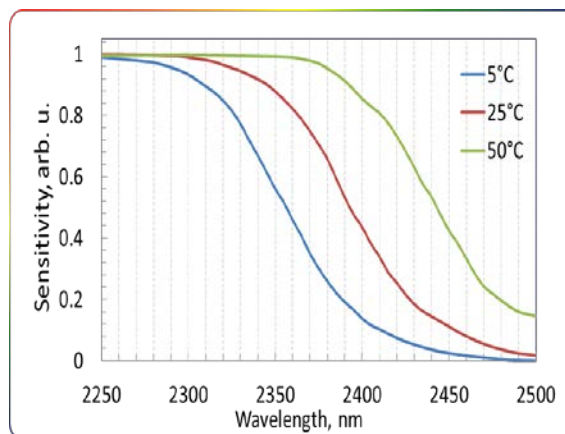

Dark current temperature dependence

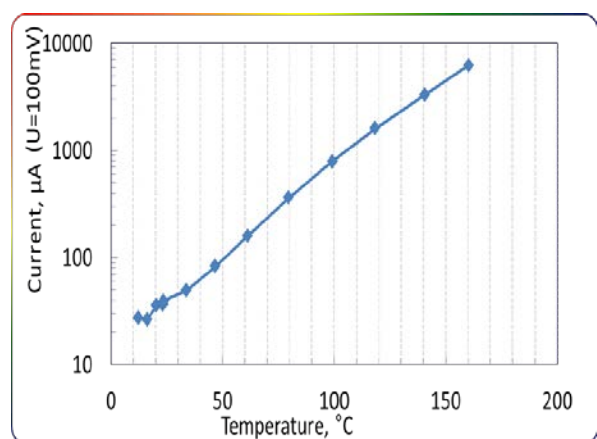


Resistance-temperature dependence

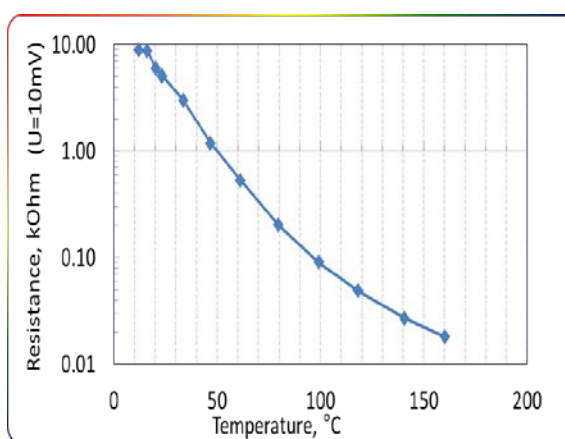

# TO18 Package with a parabolic reflector without a window

Dimension Drawing (units: mm)

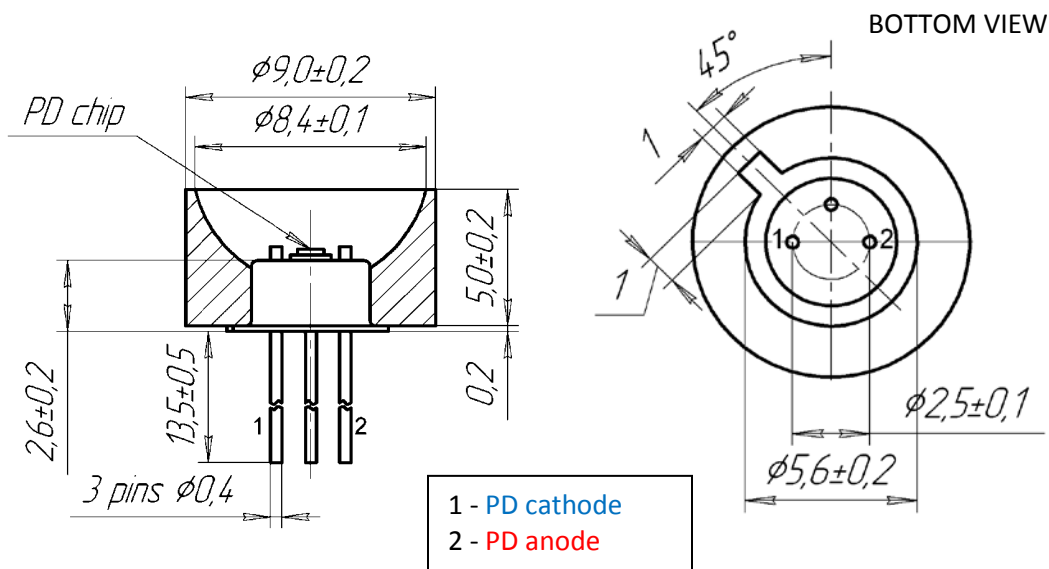

## Precautions

Photodiodes are polarity sensitive. Please note the anode of PD is marked with a RED dot. Check all polarity connections before using the device. Please do not connect the PD to the multimeter.

The MID-IR photodiodes are ESD (electro static discharge) sensitive and should be handled with the proper ESD protection environment.